

This Page Is Inserted by IFW Operations  
and is not a part of the Official Record

## **BEST AVAILABLE IMAGES**

Defective images within this document are accurate representations of the original documents submitted by the applicant.


Defects in the images may include (but are not limited to):

- BLACK BORDERS
- TEXT CUT OFF AT TOP, BOTTOM OR SIDES
- FADED TEXT
- ILLEGIBLE TEXT
- SKEWED/SLANTED IMAGES
- COLORED PHOTOS
- BLACK OR VERY BLACK AND WHITE DARK PHOTOS
- GRAY SCALE DOCUMENTS


**IMAGES ARE BEST AVAILABLE COPY.**

**As rescanning documents *will not* correct images,  
please do not report the images to the  
Image Problem Mailbox.**

1/18

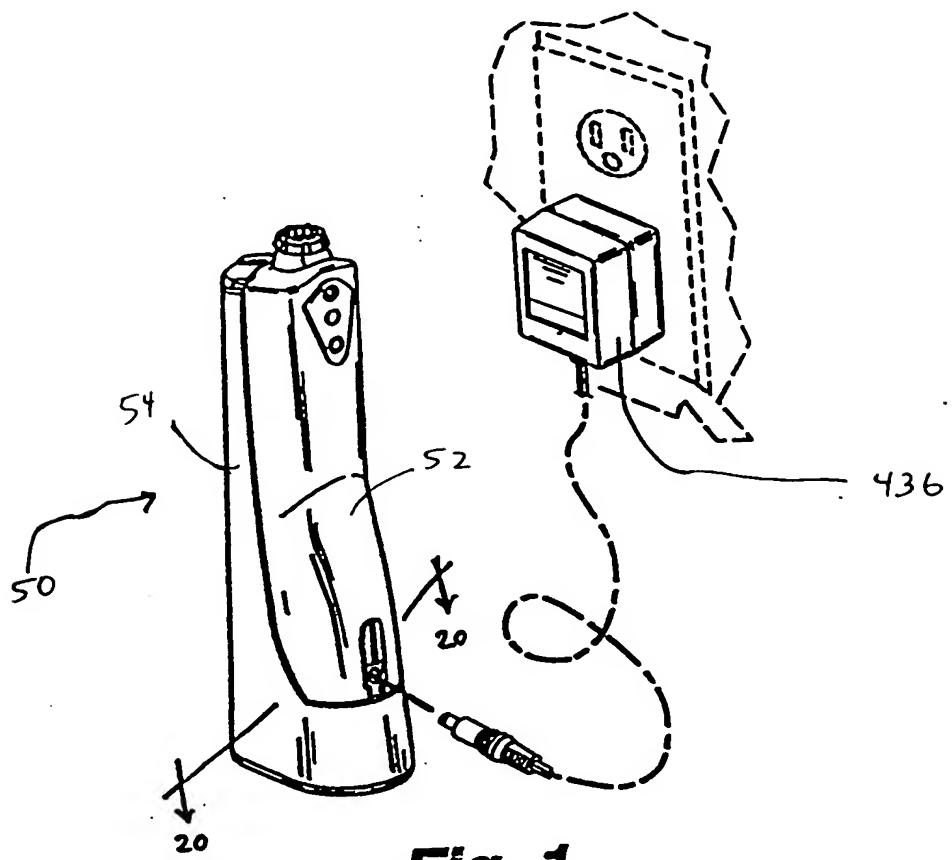


**Fig. 1**

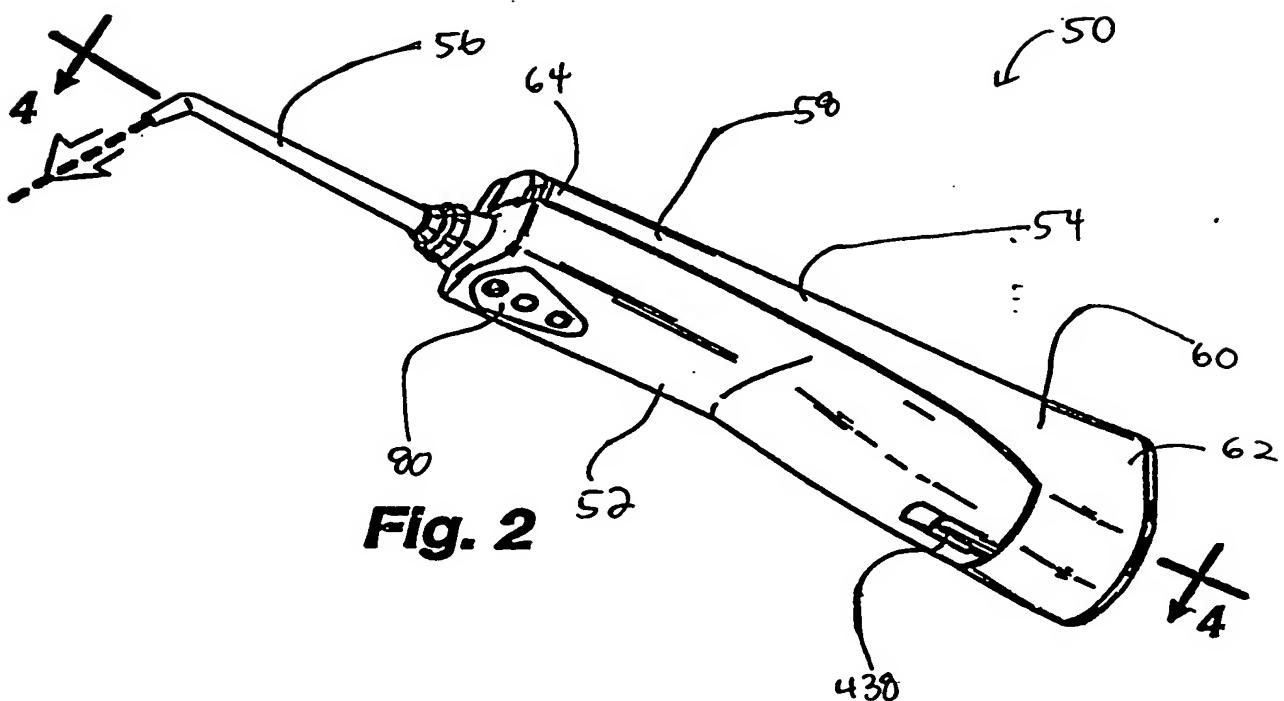


**Fig. 2**

2/18

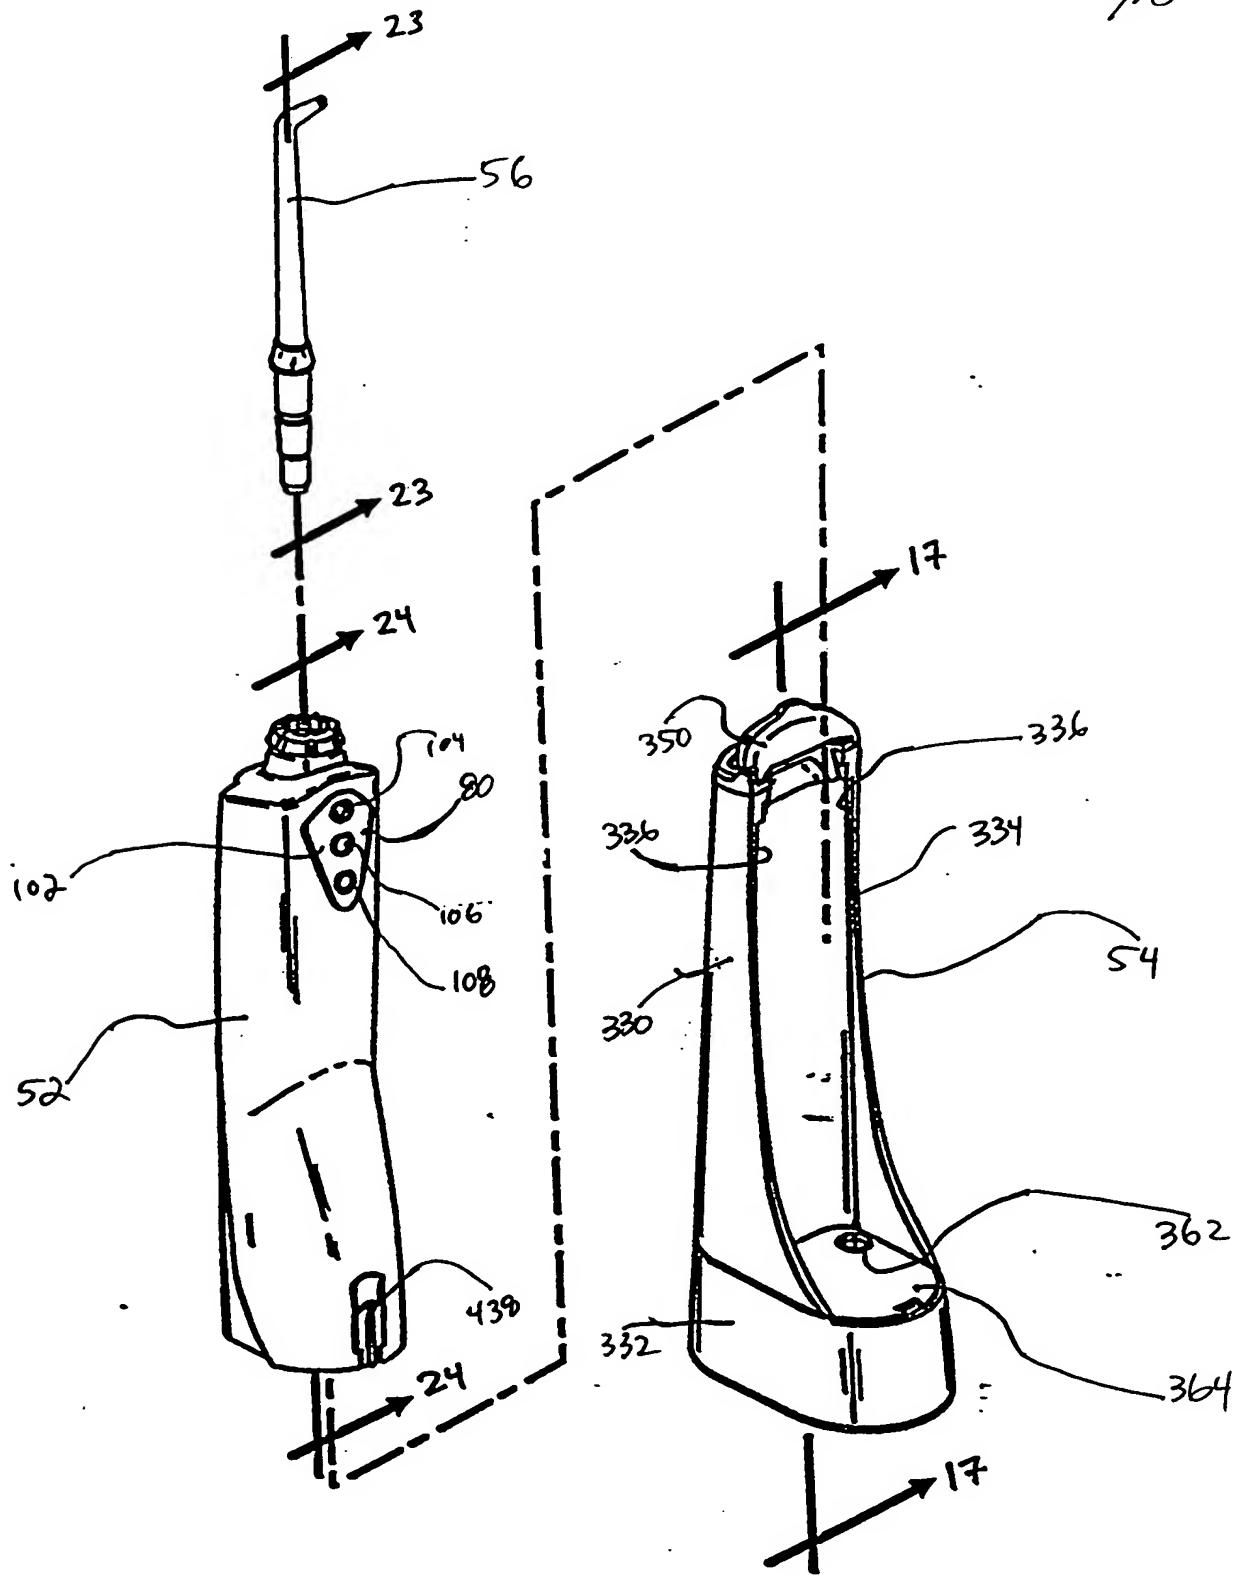

**Fig. 3**

3/18

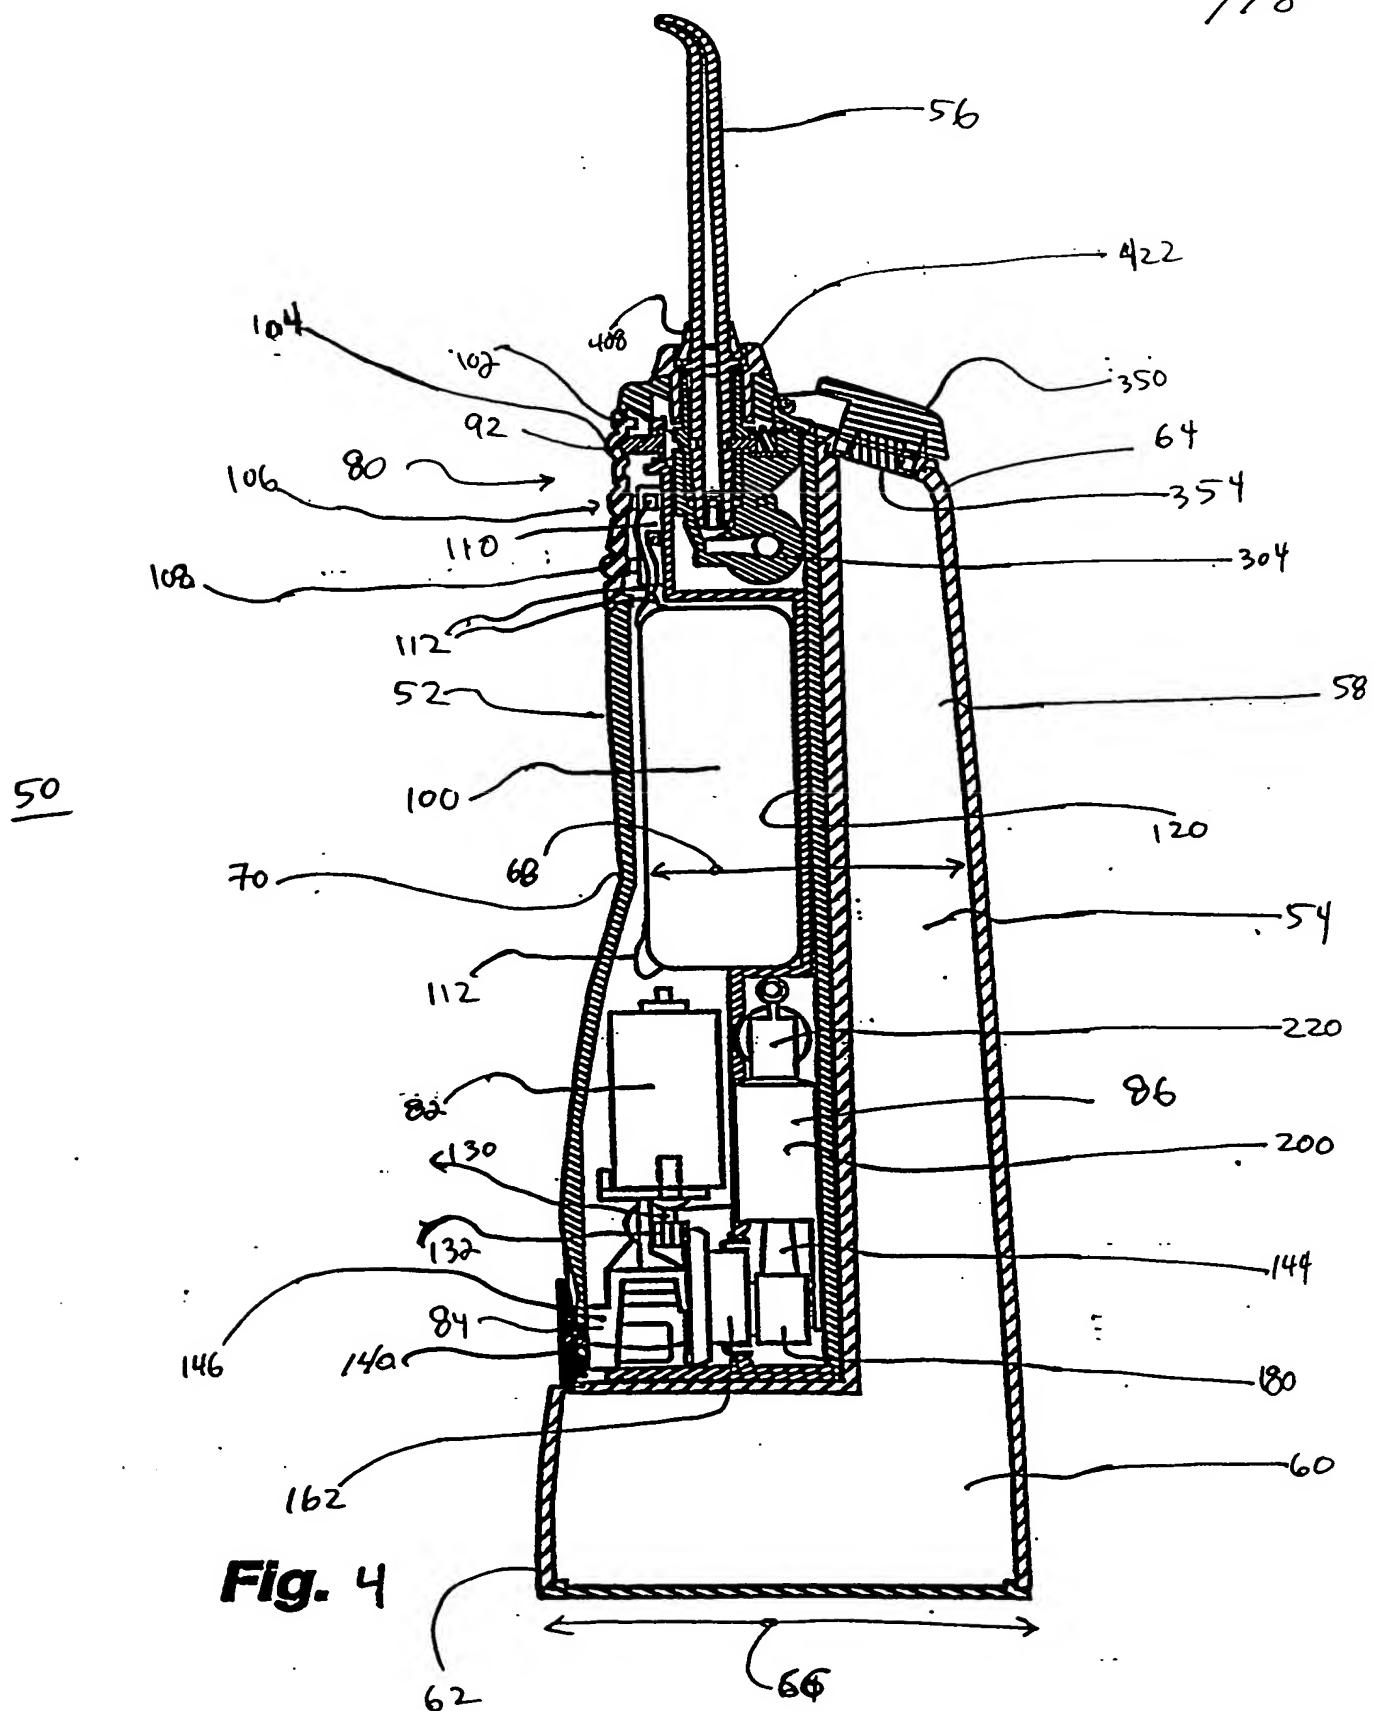

4/18

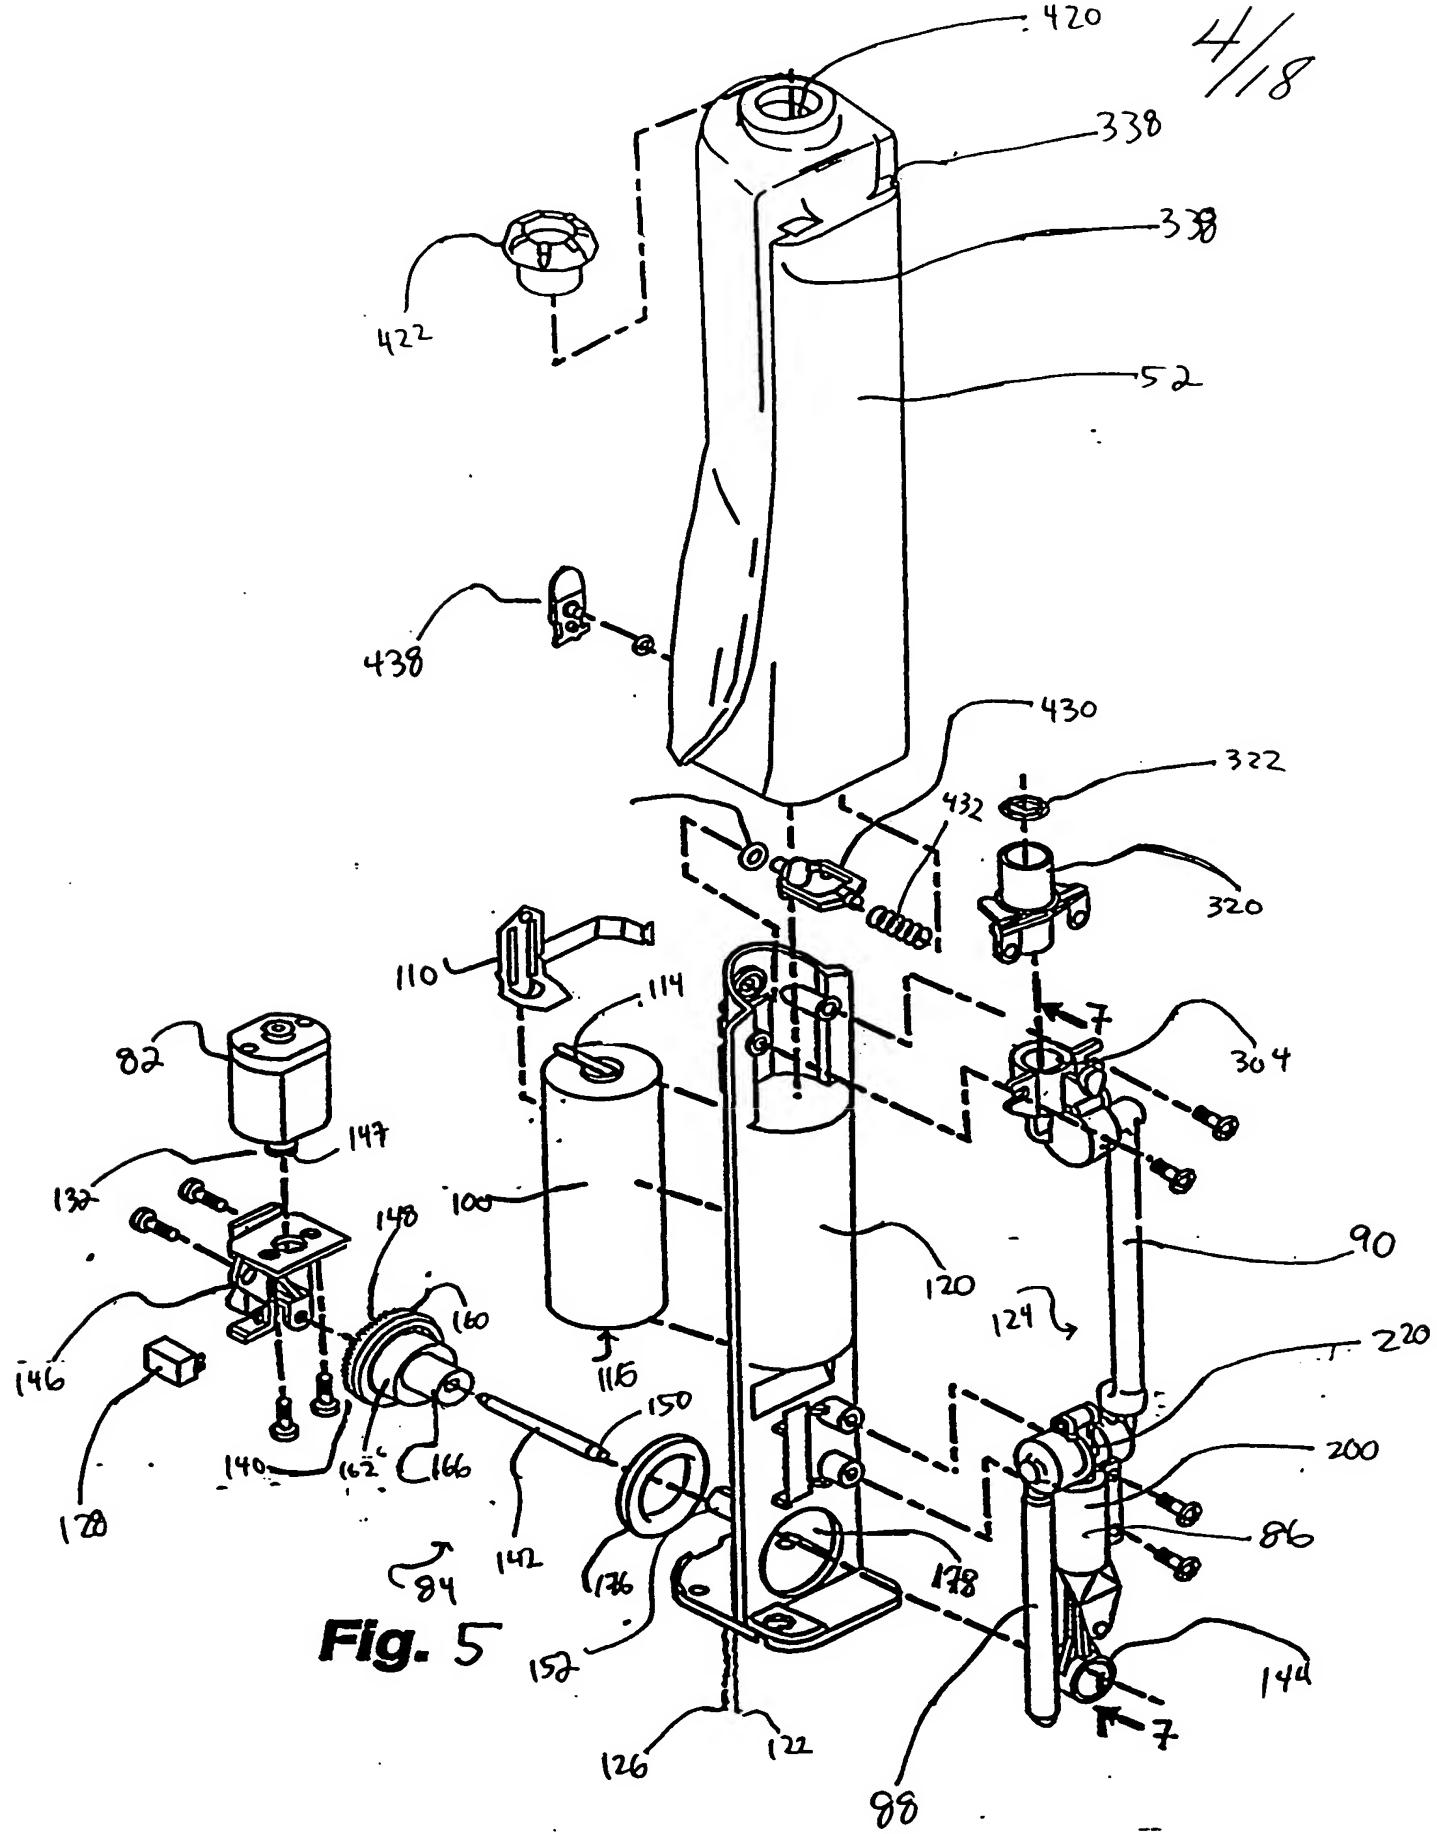


Fig. 5

5/18

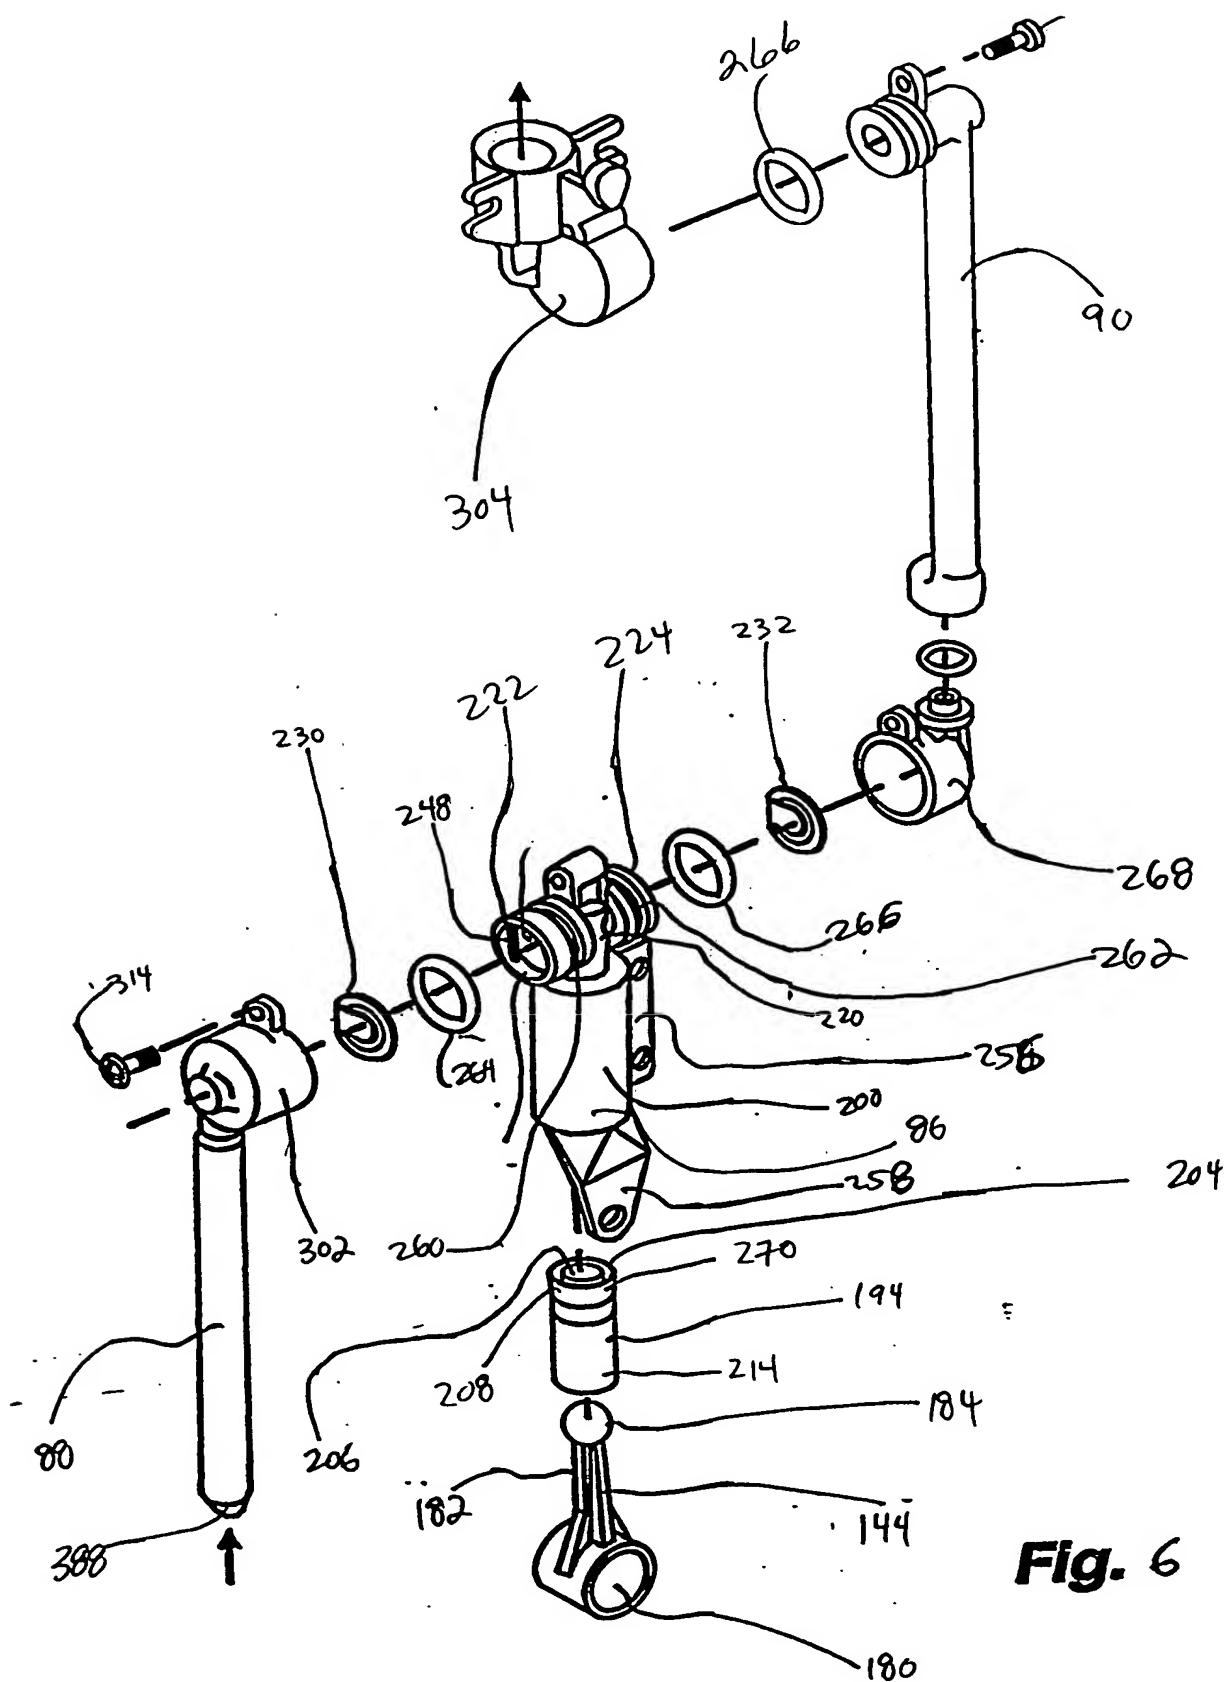


Fig. 6

6/18

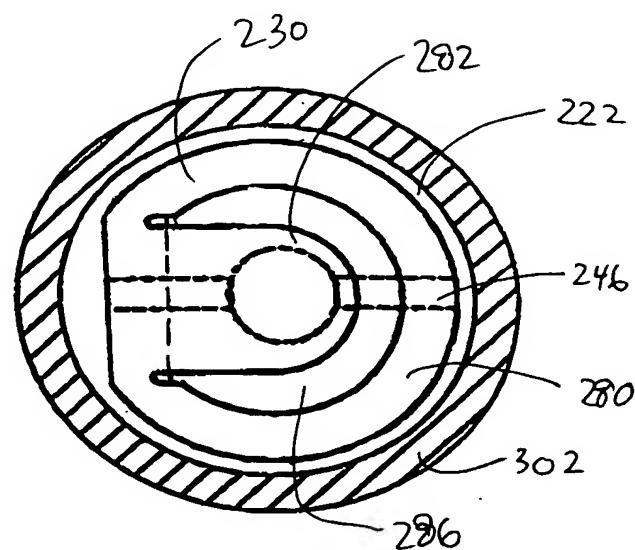
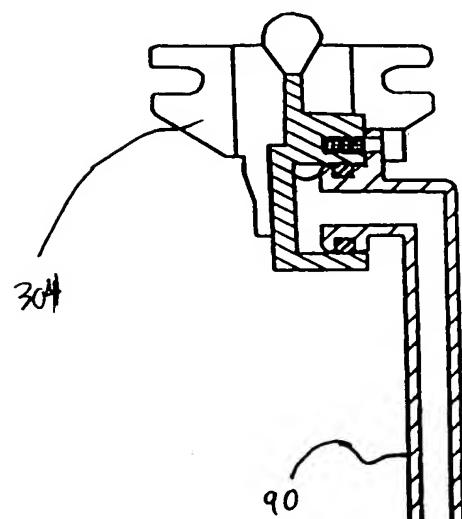


Fig. 9

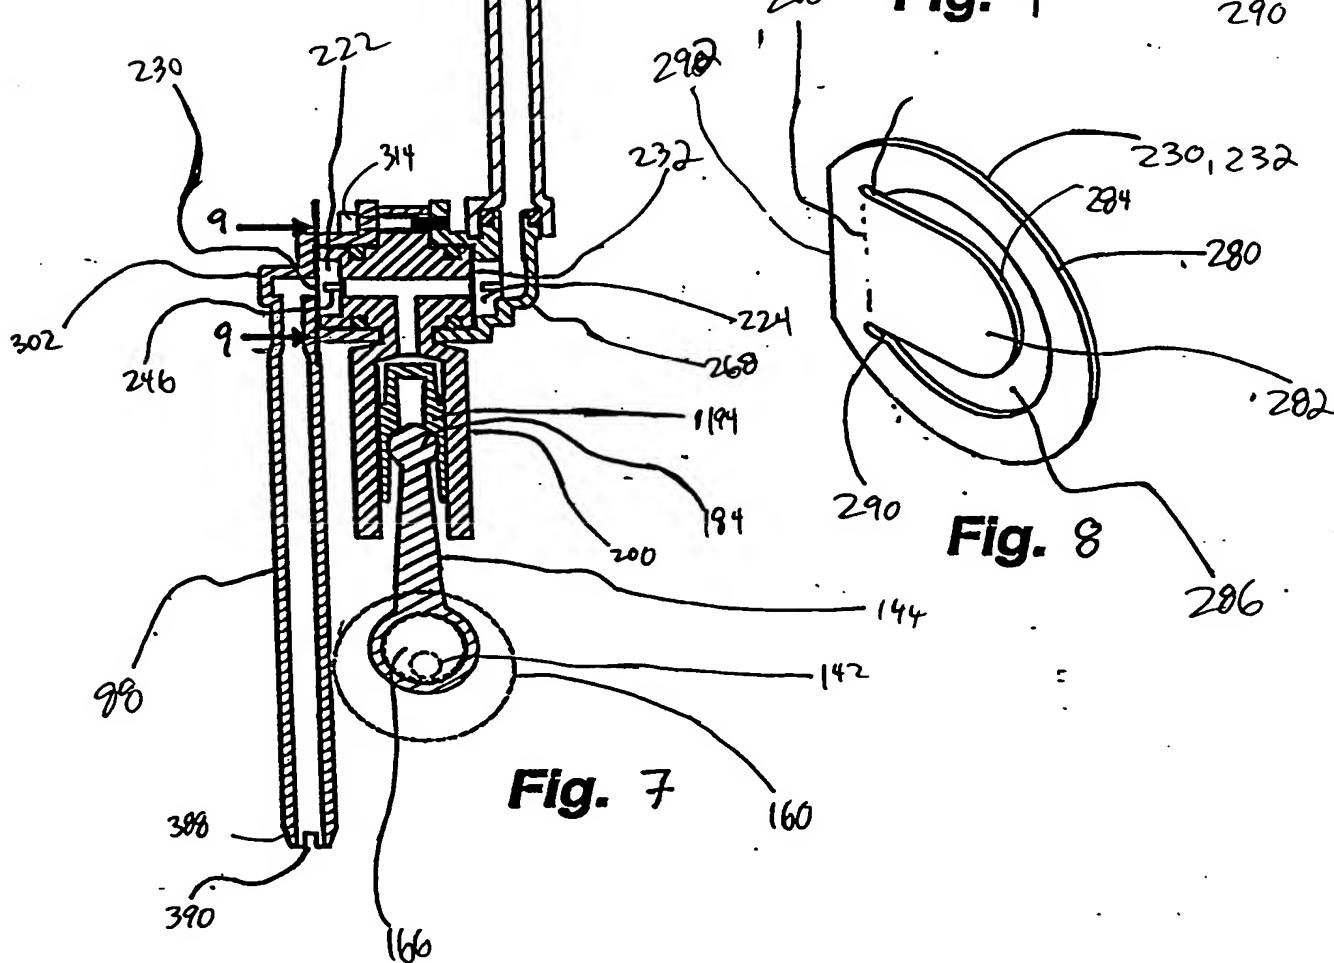
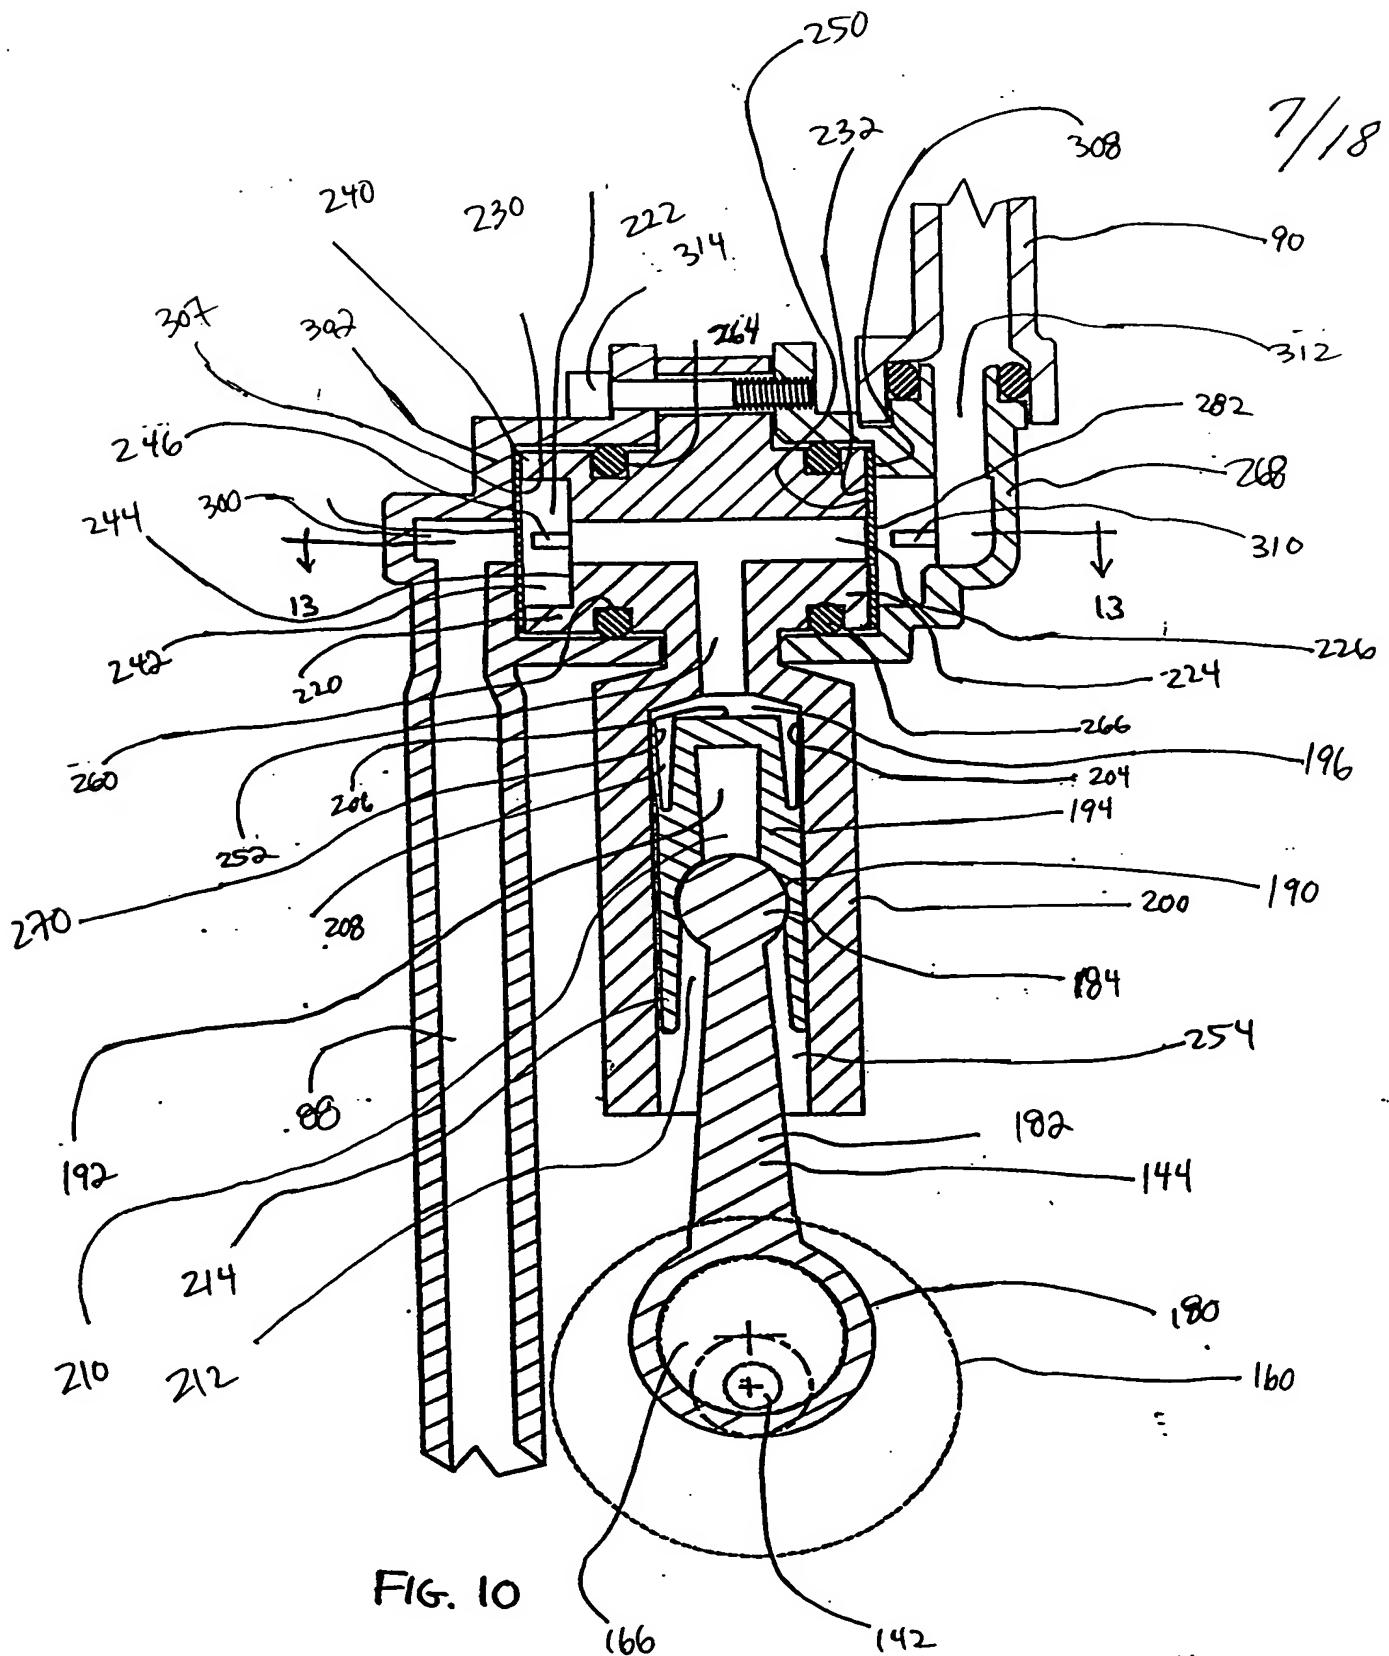


Fig. 7

Fig. 8

**HAND HELD ORAL IRRIGATOR, non-provisional of 60/437,300, filed herewith, Attorney Docket No. 1985/US/2, PH 303-629-3400**



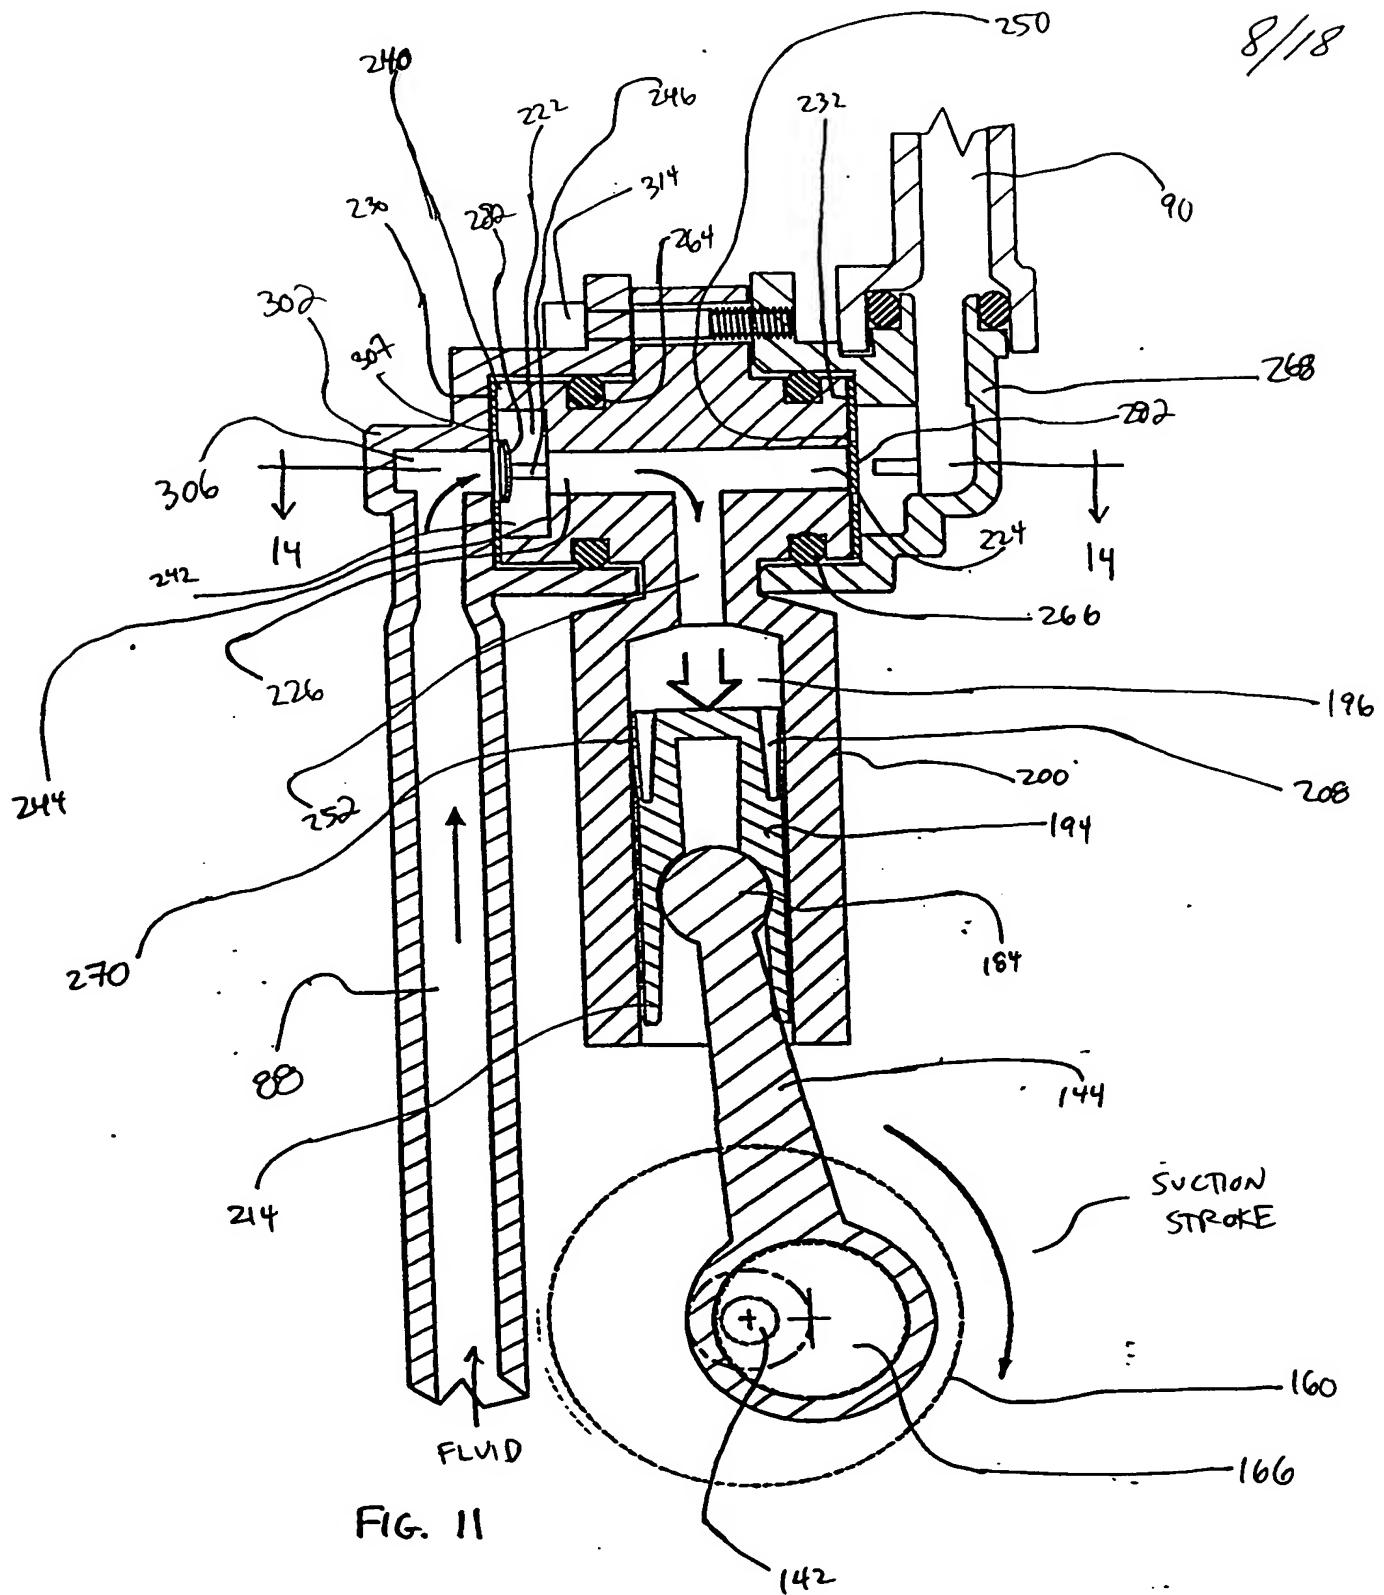


FIG. II

9/18





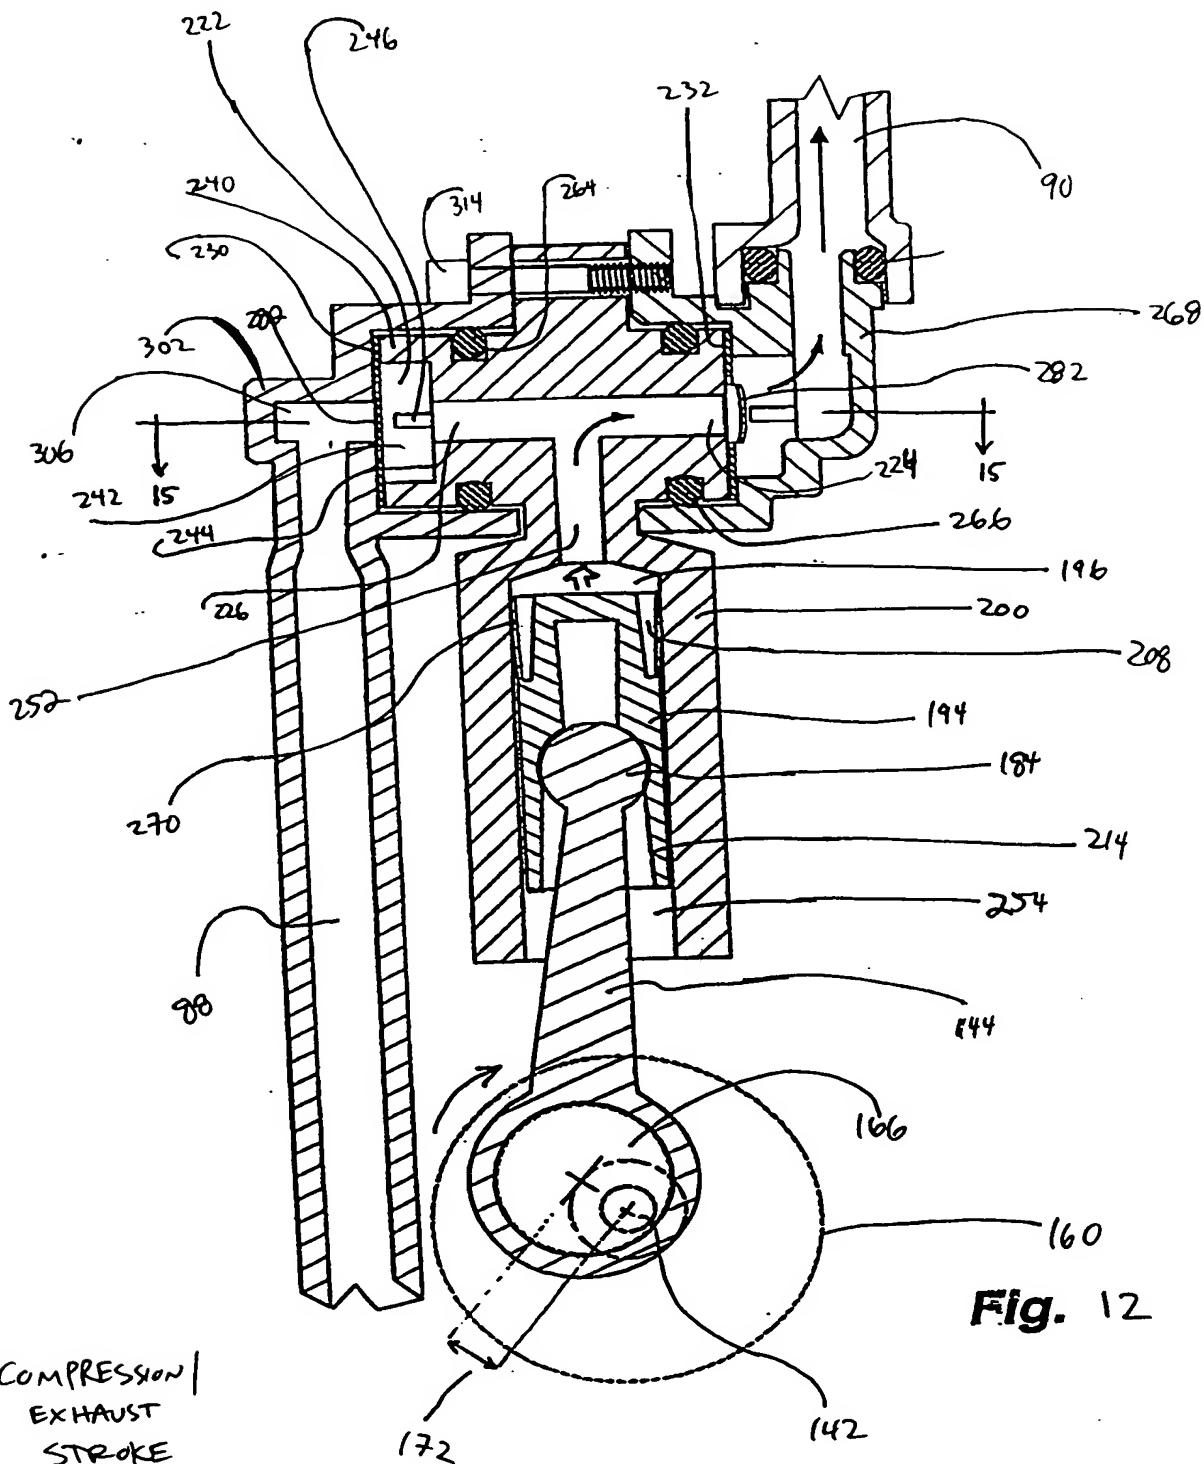


Fig. 12


## COMPRESSION EXHAUST STROKE

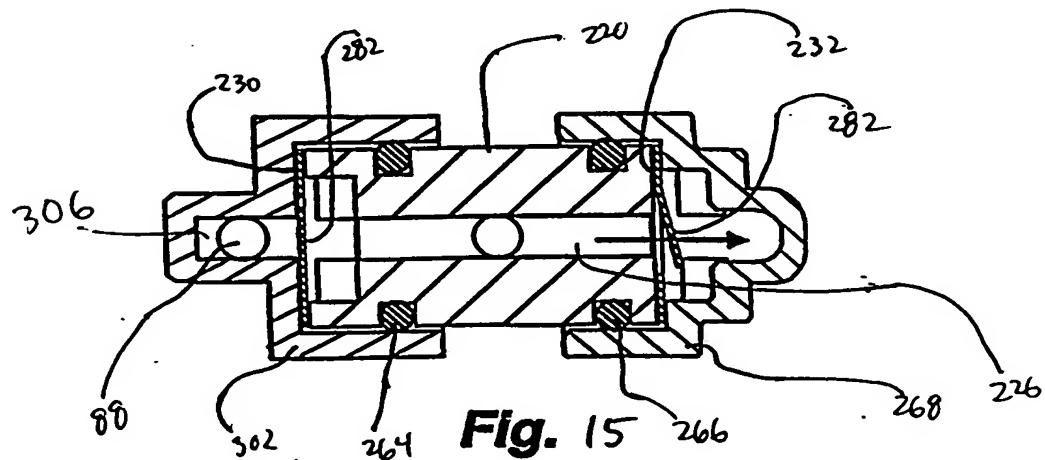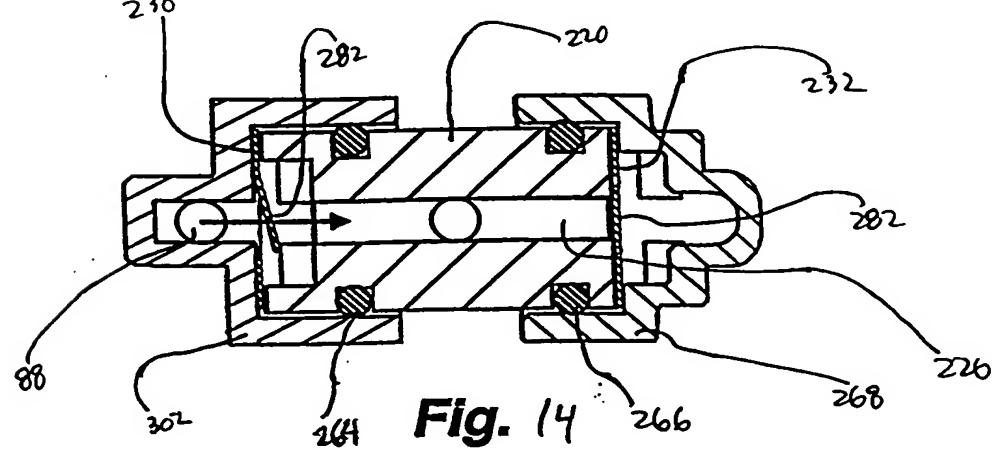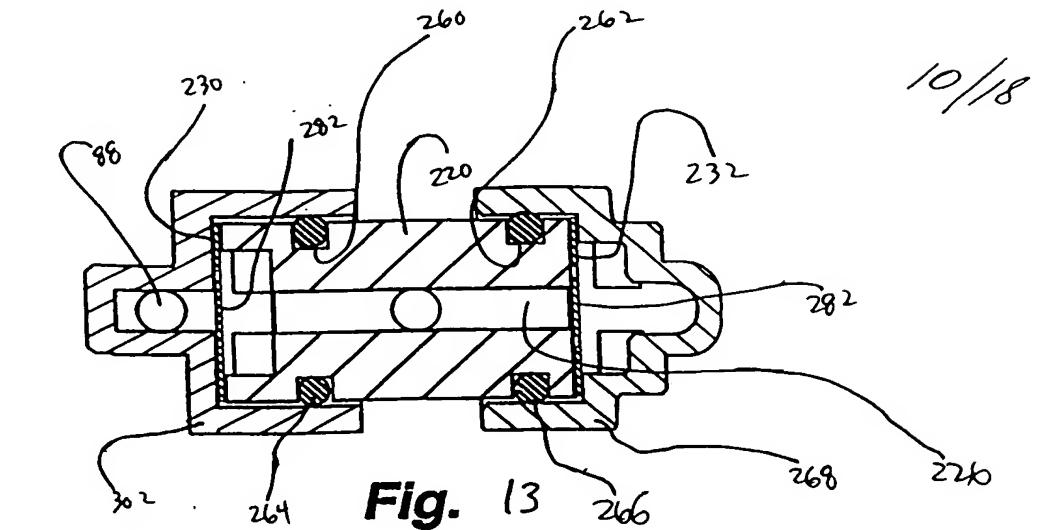


11/18

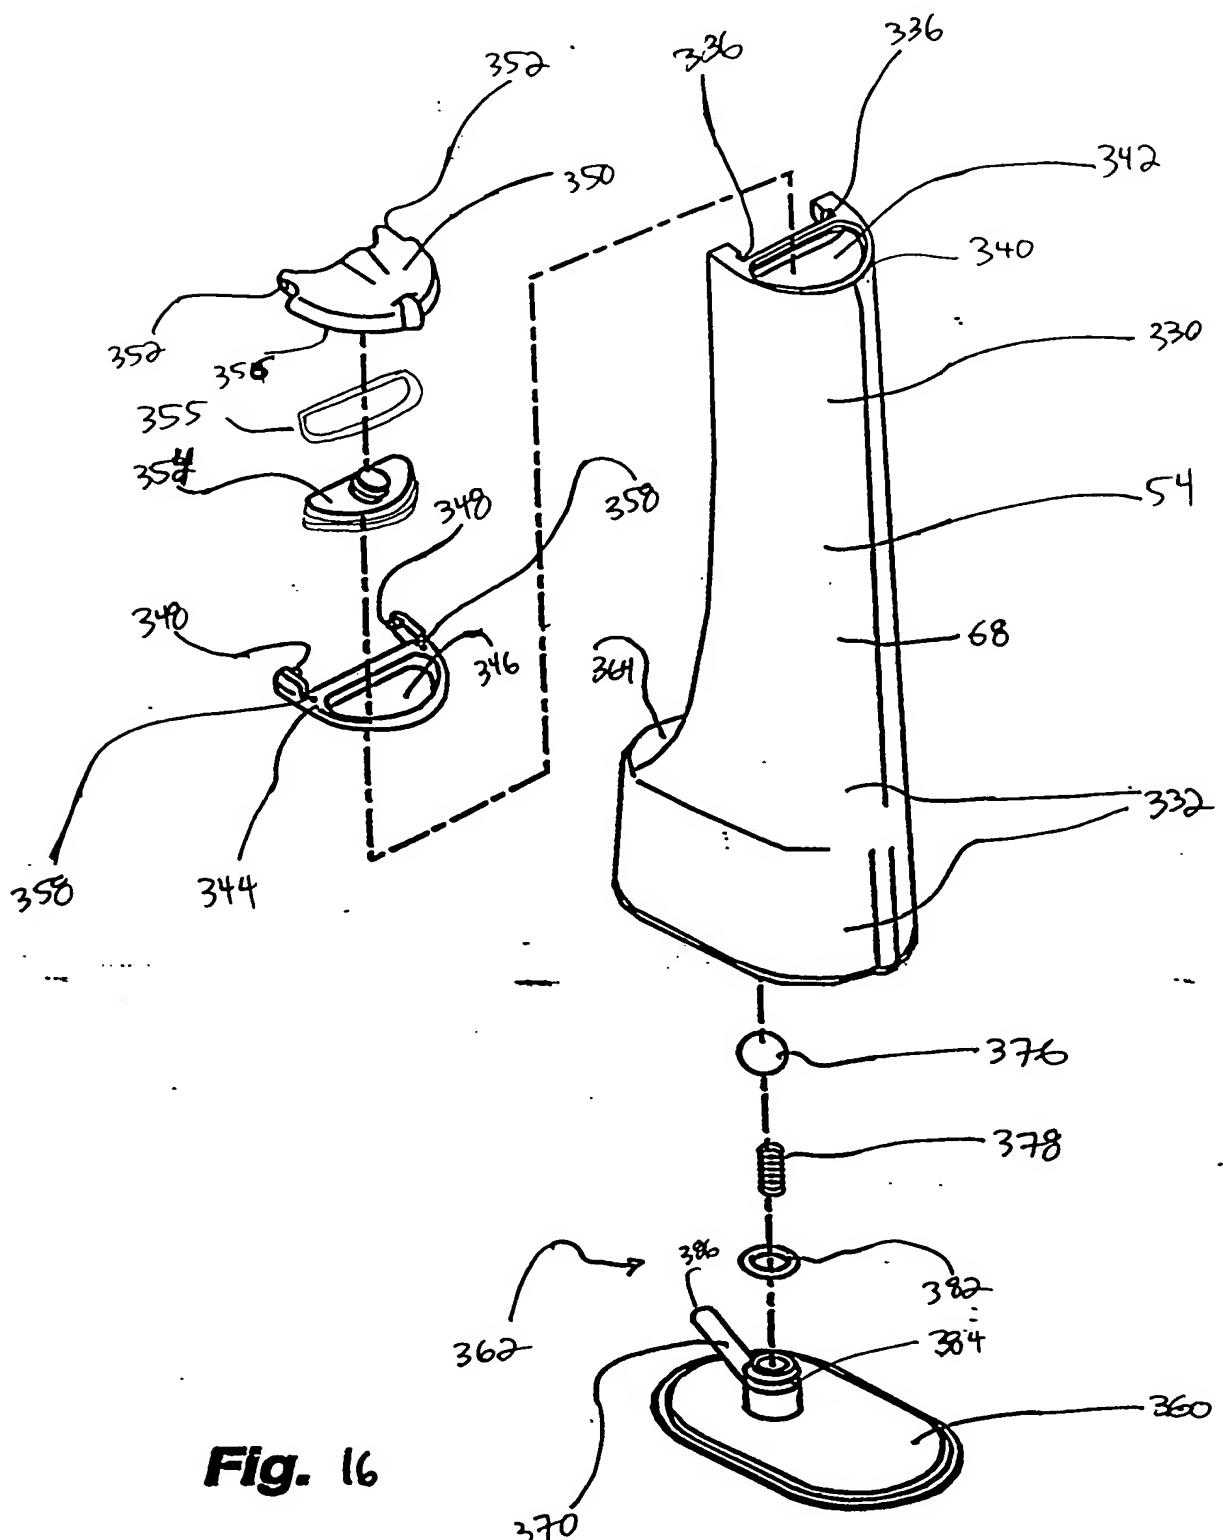

**Fig. 16**

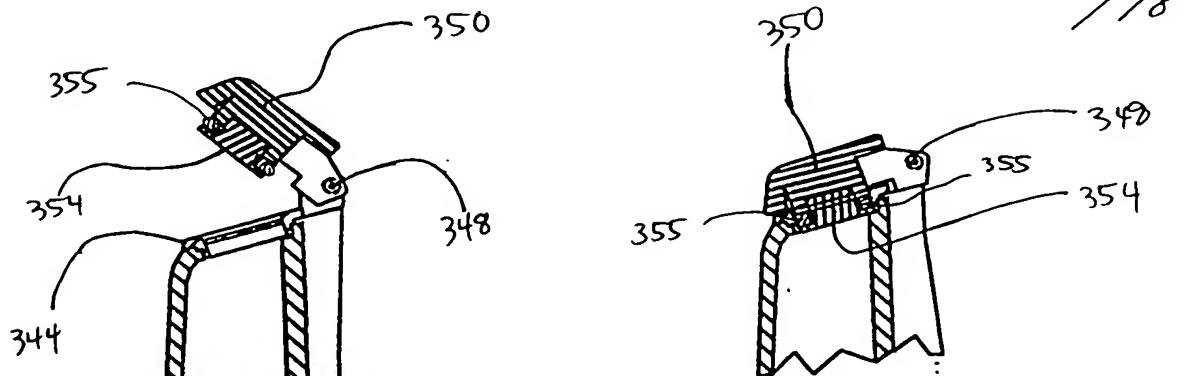


**Fig. 18**

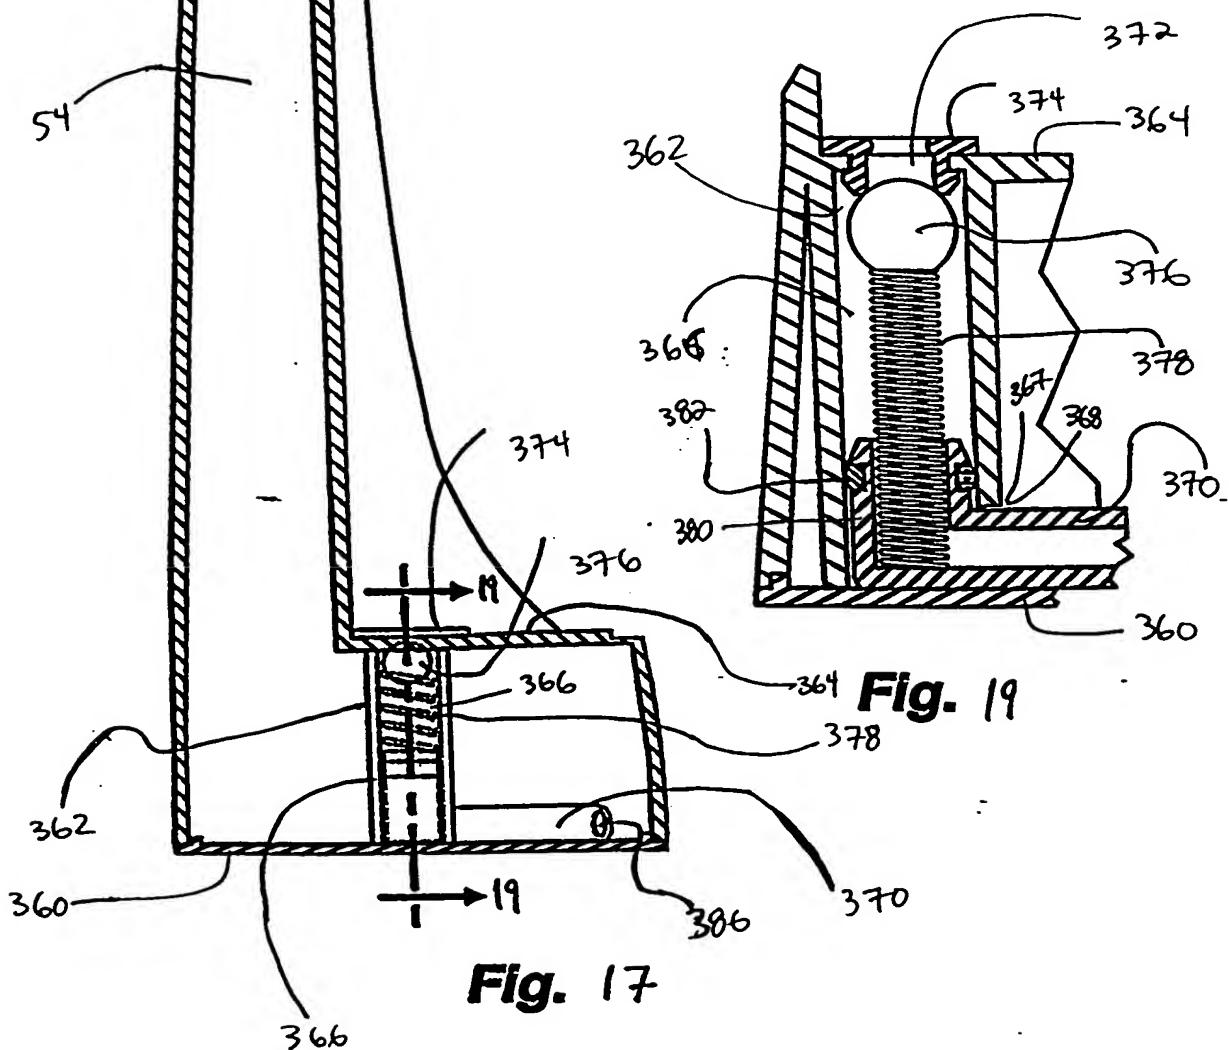


**Fig. 17**

13/18

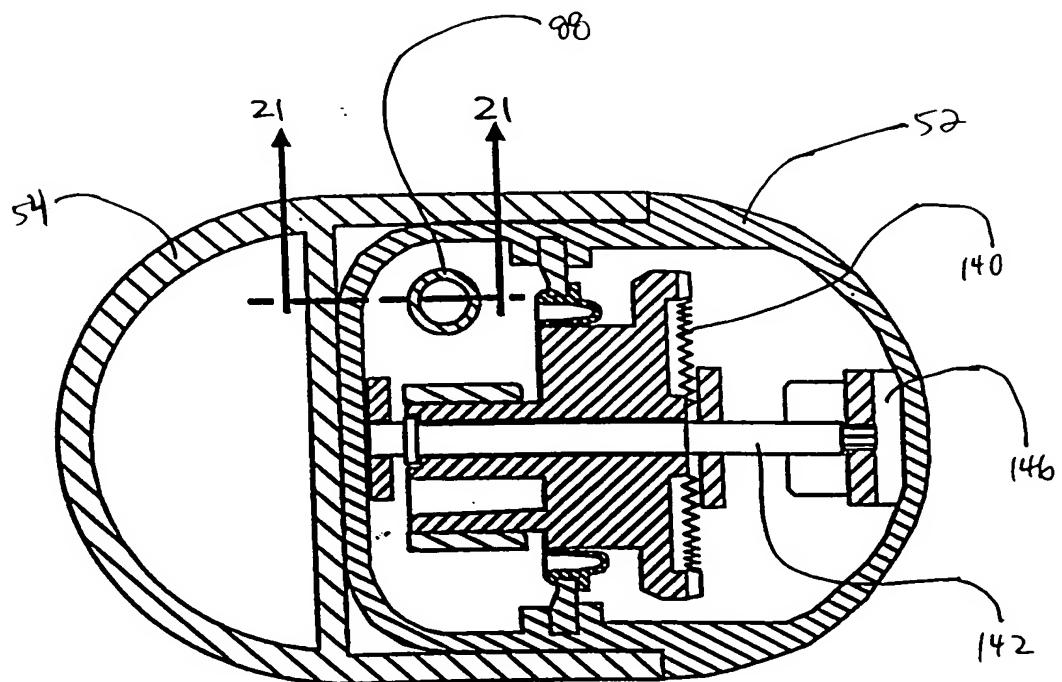


**Fig. 20**

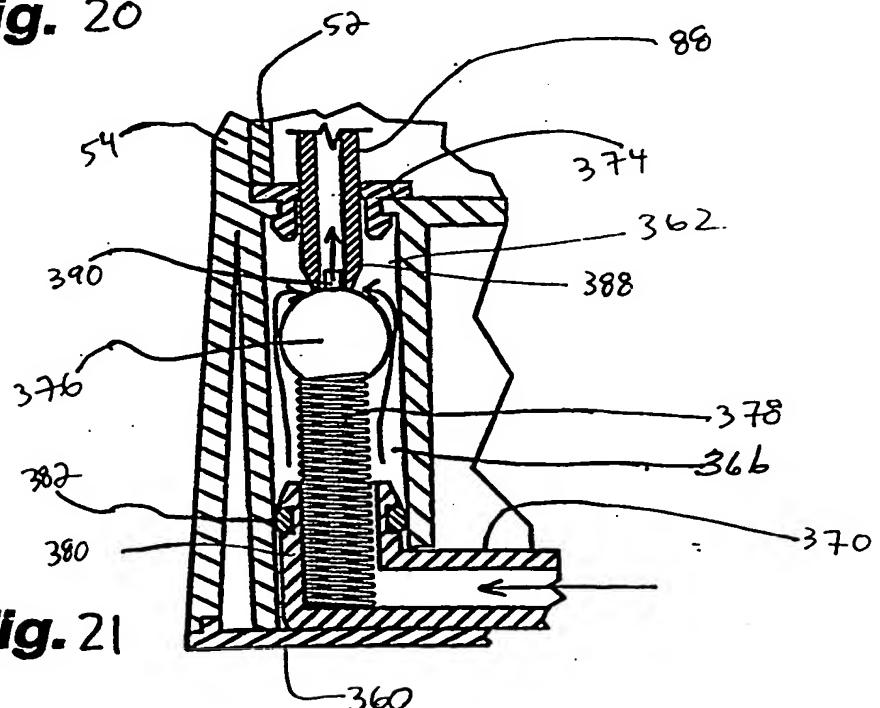



**Fig. 21**

14/18

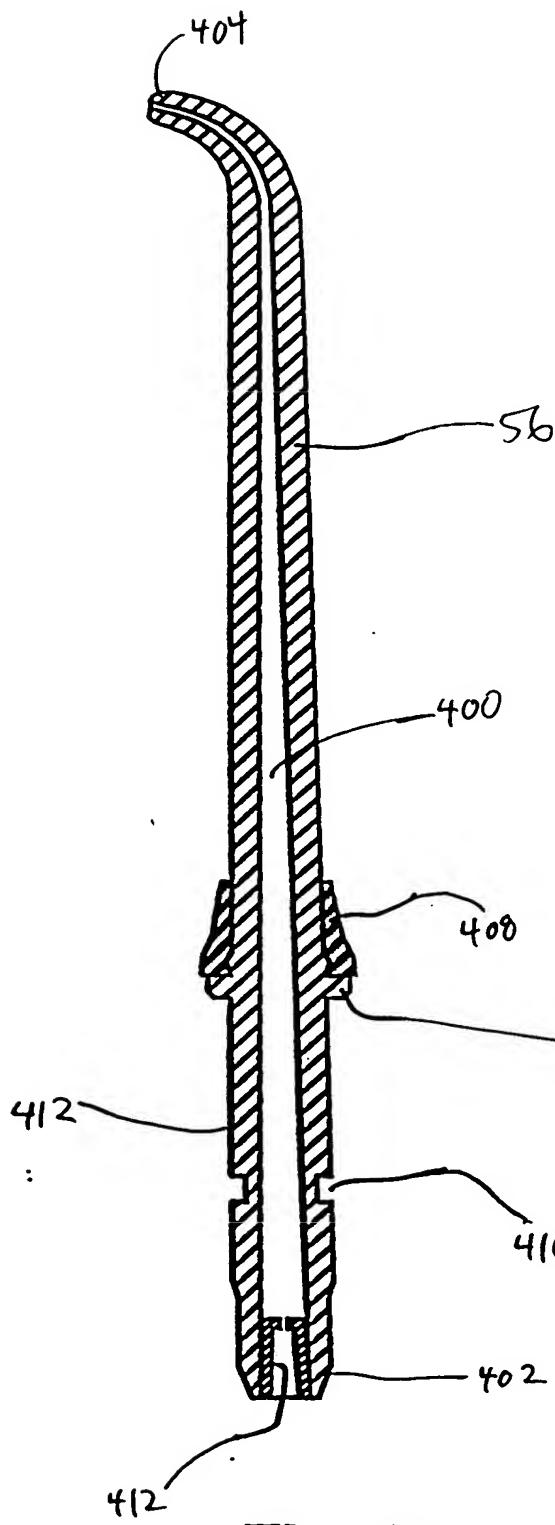

**Fig. 23**

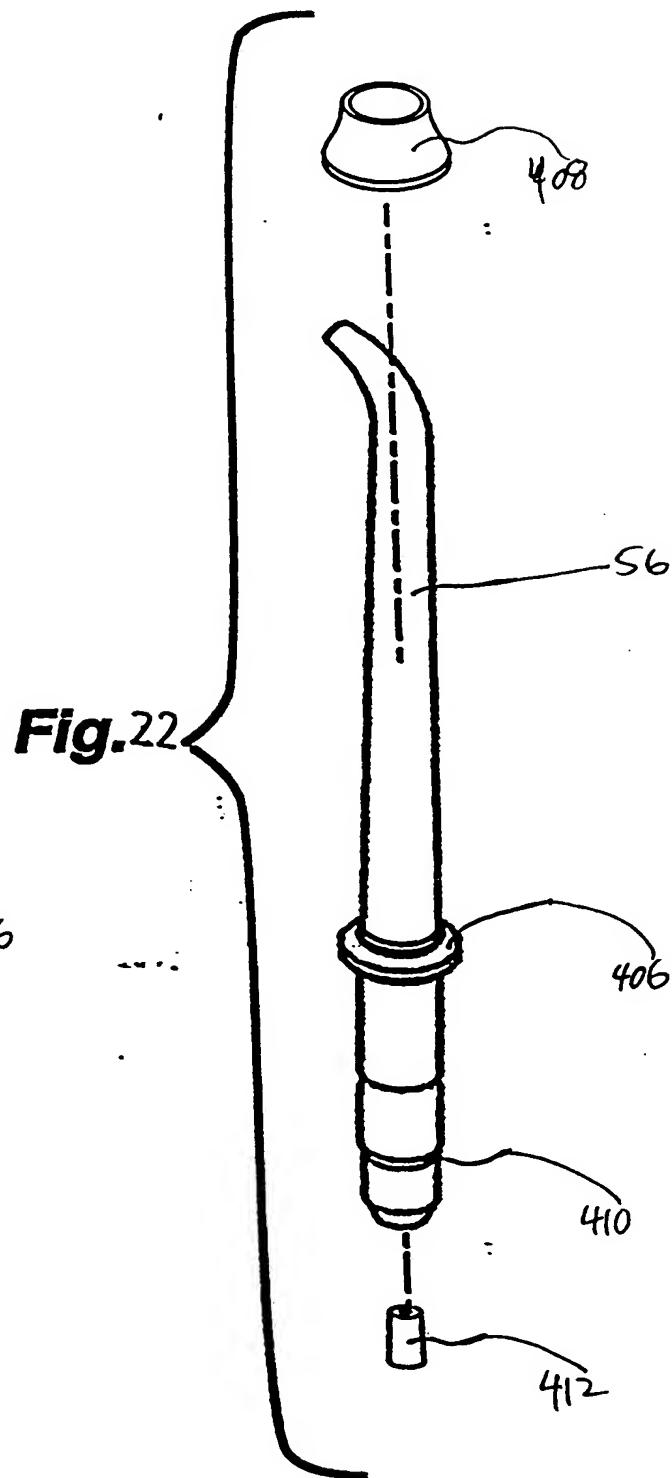

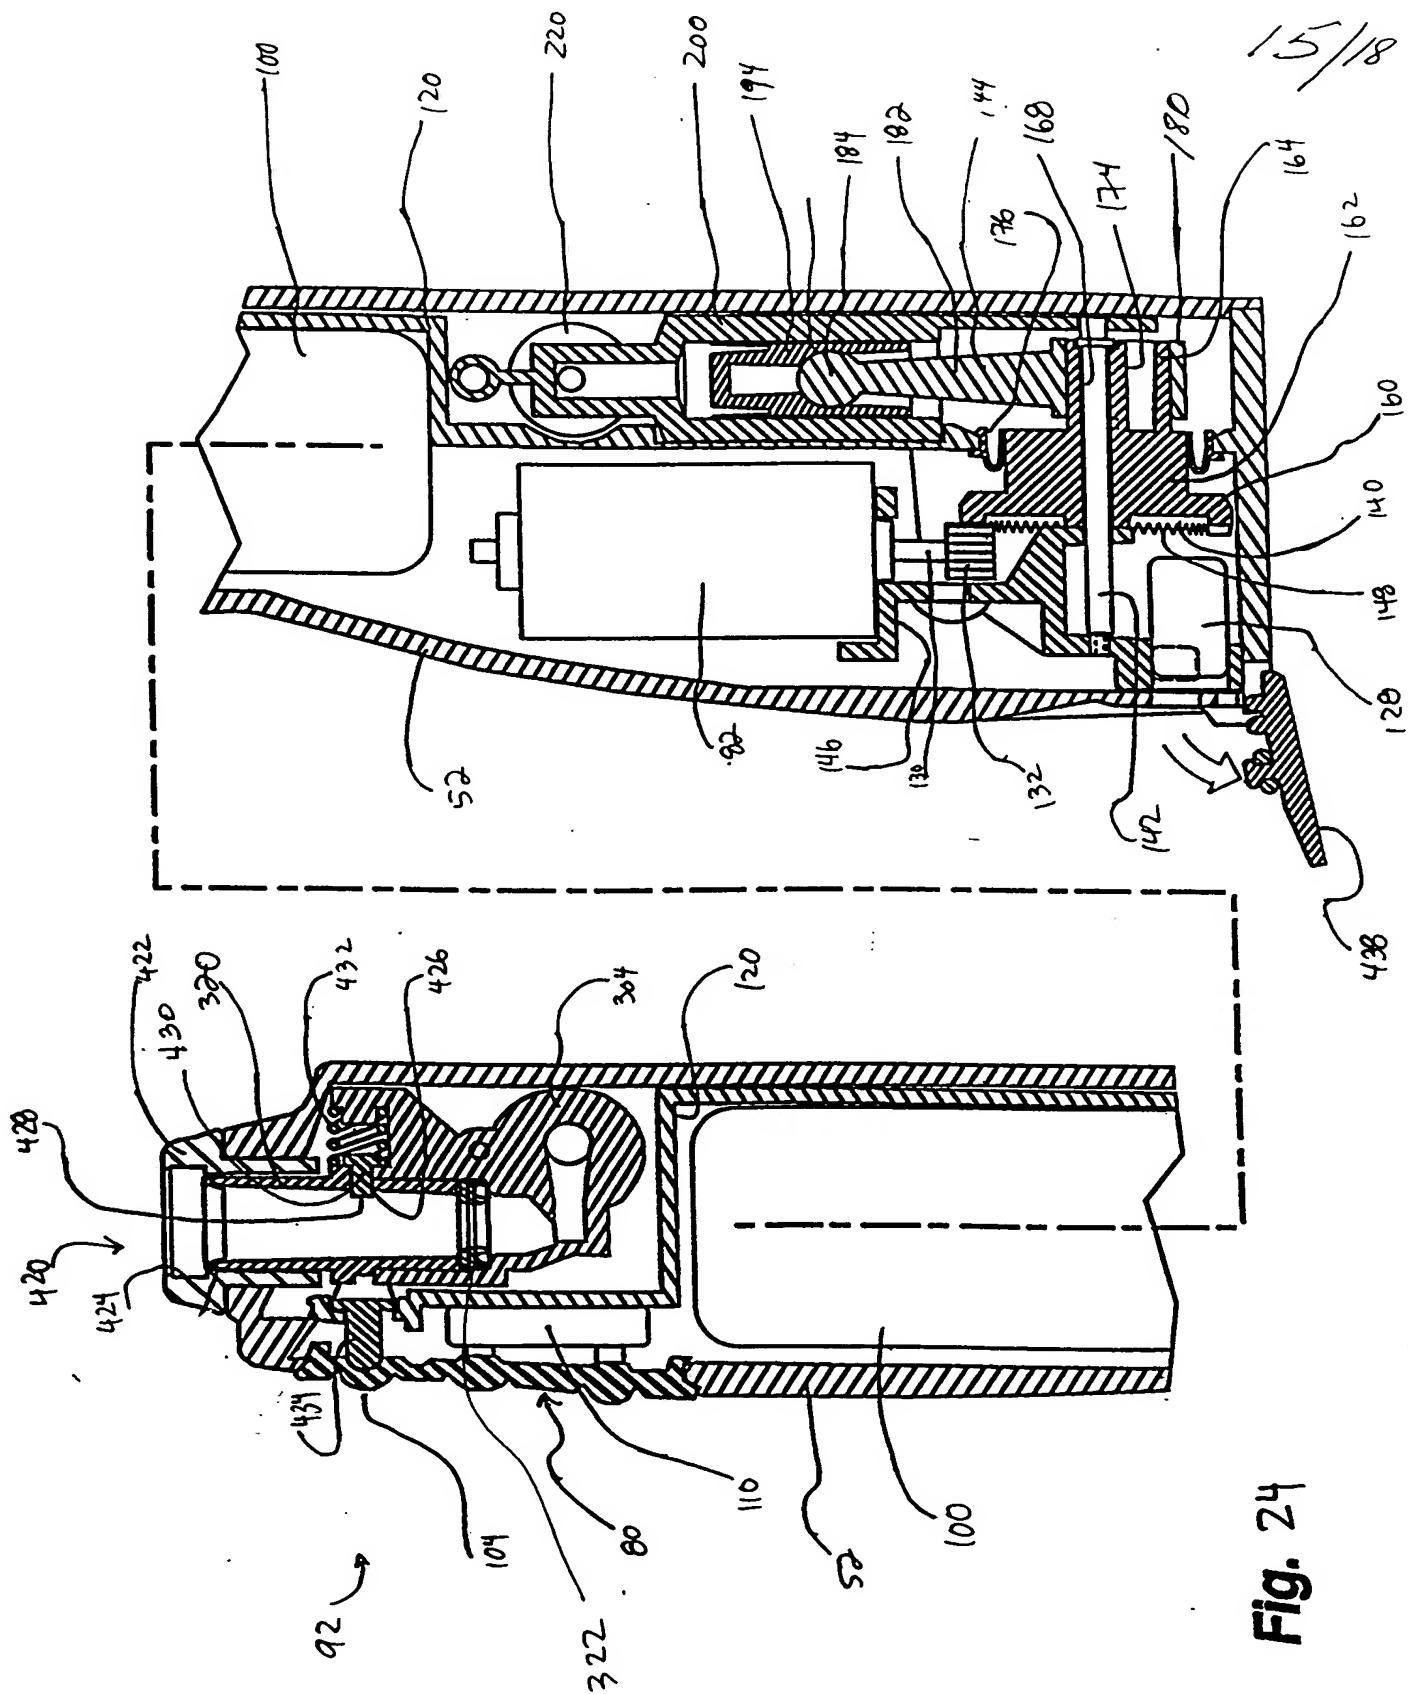

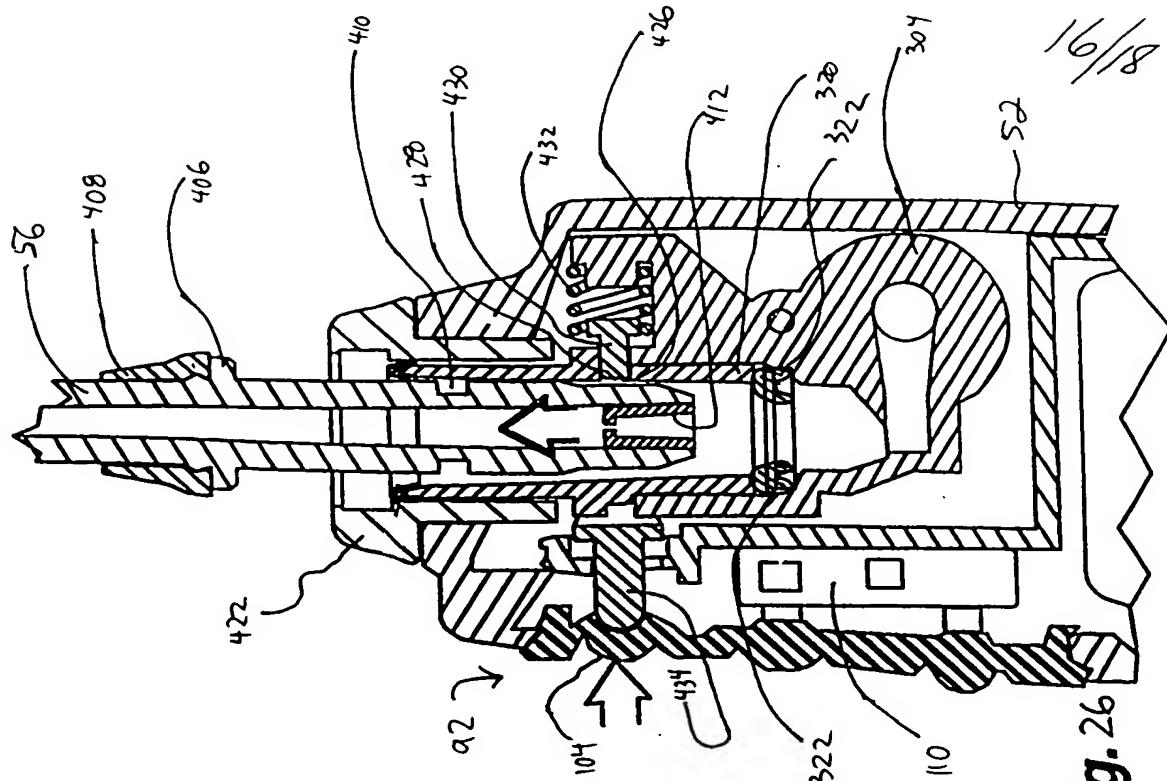


Fig. 26

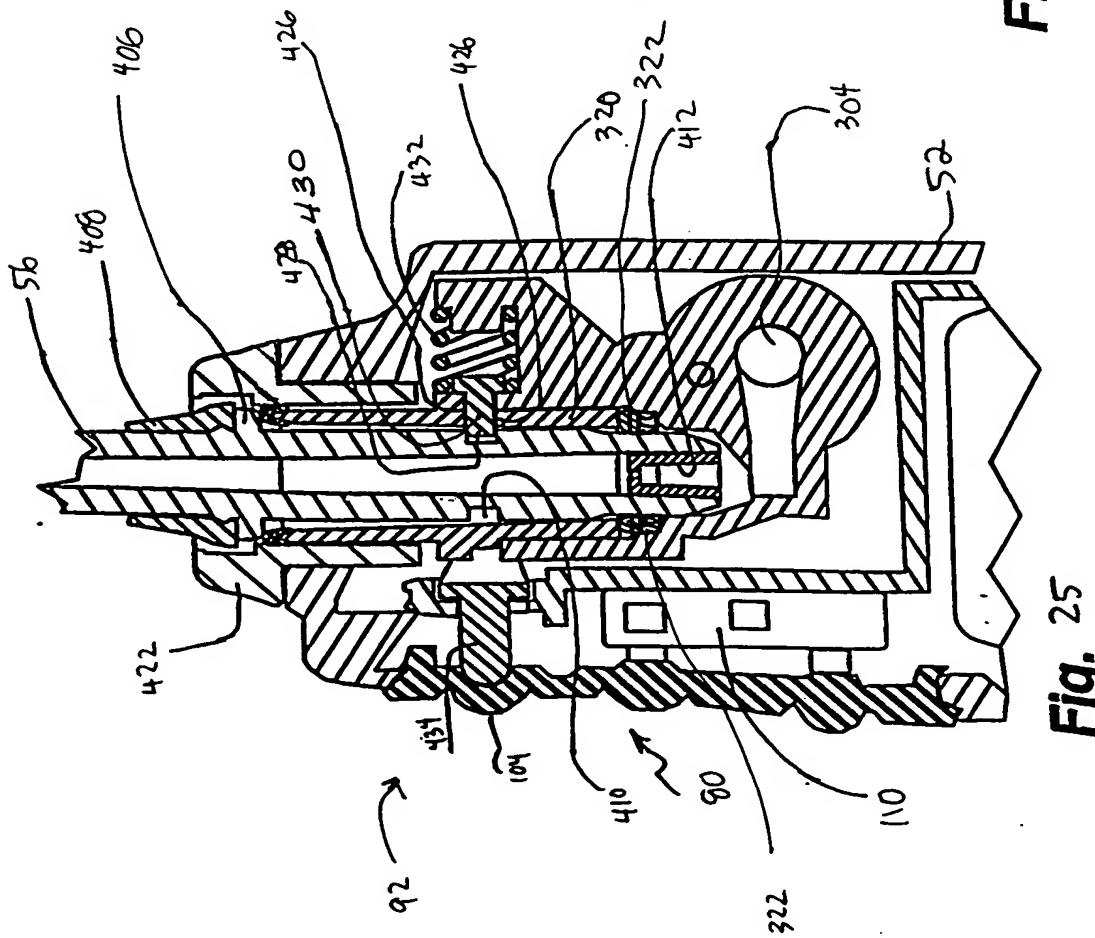
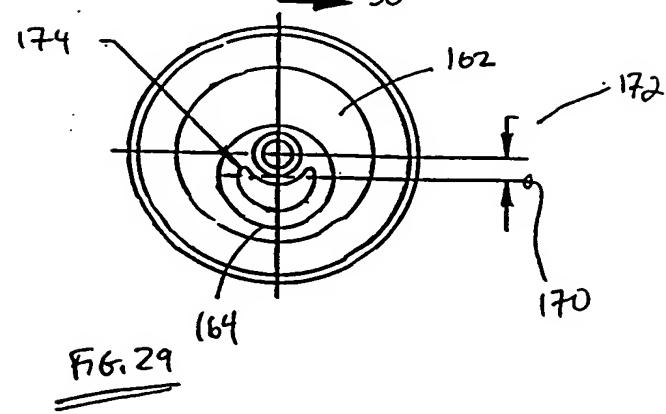
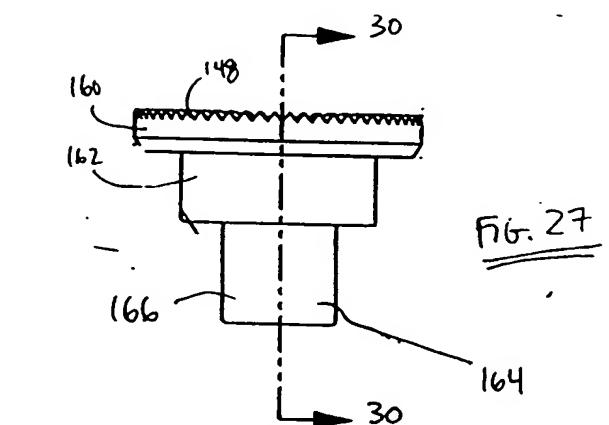
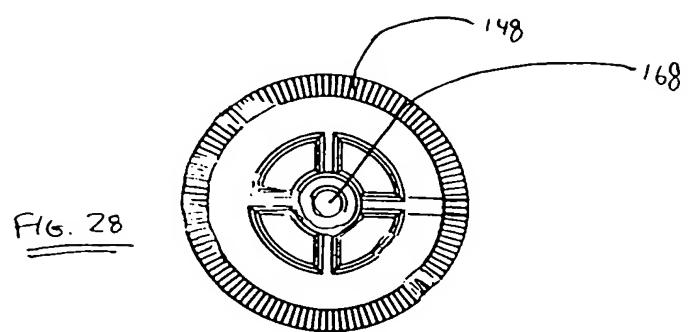
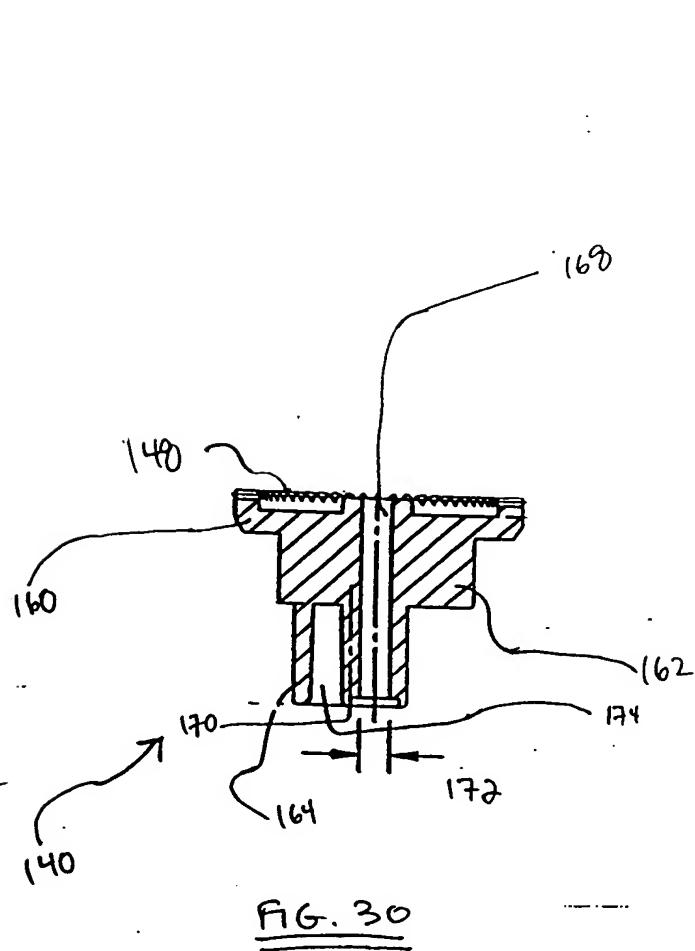


Fig. 25

17/18



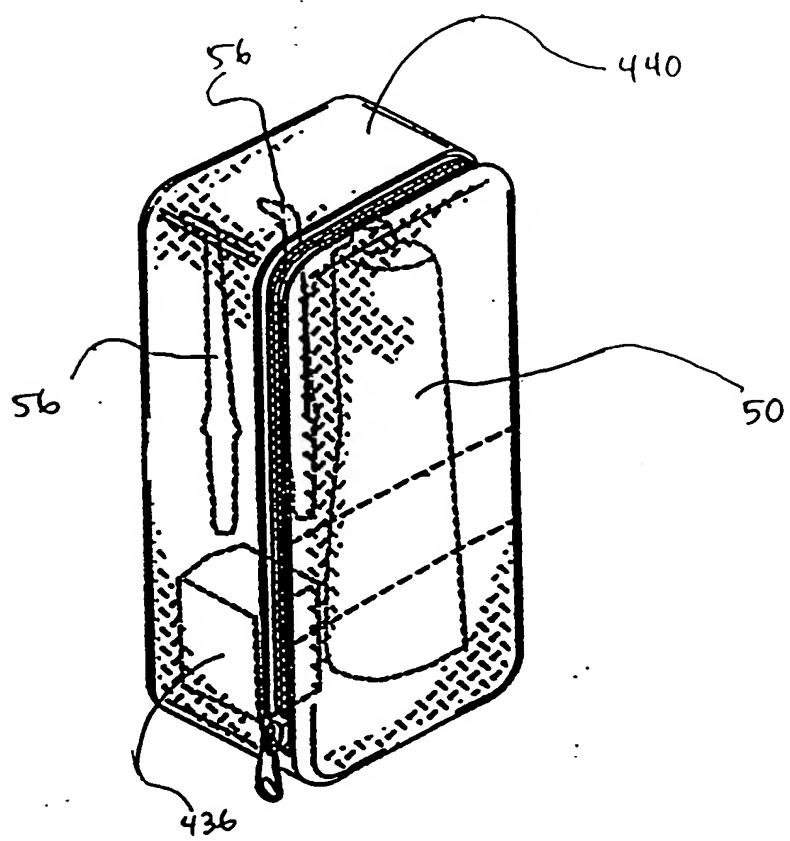


Fig. 31